



Malate Assay (Mal)

Cat. No. 8648
100 Tests in 96-well plate

Introduction

L-Malate (Mal) is a tricarboxylic acid cycle intermediate and a critical component of the malate-aspartate shuttle. Malate also improve muscle performance and act as a metal chelator. In plants, malate is a source of CO₂ for the Calvin Cycle in the C₄ carbon fixation process. Malate is frequently used as an additive in the food and pharmaceutical industries. This colorimetric assay is based on malate dehydrogenase-catalyzed oxidation of malate, where the resulting NADH can then convert a nearly colorless probe to a colored product; the intensity of the colored product is proportional to the amount of malate in the sample, exhibiting maximum absorbance at 440nm.

Kit Components

Cat. No.	# of vials	Reagent	Quantity	Storage
8648a	1	Assay buffer	25 mL	4°C
8648b	1	Malate standard	0.5 mL	-20°C
8648c	1	Developer (10X)	0.1 mL	-20°C
8648d	1	NAD	0.5 mL	-20°C
8648e	1	WST	3.91 mg	-20°C
8648f	1	Cofactor	0.5 mL	4°C
8648g	1	Enzyme	0.1 mL	-20°C

Product Use

The Malate Assay kit measures the malate level in different types of samples, including tissue and cell lysate. This product is for research purposes only and is not for use in animals, humans, or diagnostic procedures.

Quality Control

Data from Malate Assay kit measuring malate solutions with concentrations ranging from 0.00625 to 0.1 mM show a linear relationship between OD_{440nm} and malate concentration (Figure 1).

Shipping

Shipped on dry ice.

Reagents preparation

1. Developer solution (1X): dilute developer (10X) (8648c) in assay buffer (8648a) (1:10).
2. WST solution: reconstitute each vial of WST with 0.6 mL assay buffer (8648a). Vortex briefly and keep in the dark at -20°C until use. For longer storage, we suggest that you aliquot and store the reconstituted WST solution at -20°C, avoid repeated freeze/thaw cycles.
3. Diluted malate standard: Add 1 µL malate standard (8648b) into 99 µL assay buffer (8648a).

Procedure (96-well plate)

A. Preparation of malate standard

1. Add 25 µL of diluted malate standard to 100 µL of assay buffer (8648a) to make a 125 µL solution of 0.2 mM malate.
2. Obtain 6 test tubes, add 110 µL of assay buffer (8648a) into each tube and label them #1 through #6.
3. Add 110 µL of the 0.2 mM malate solution into tube #1 and mix well to obtain the 0.1 mM malate standard.
4. Transfer 110 µL of the 0.1 mM malate standard from tube #1 to tube #2 and mix well to obtain the 0.05 mM malate standard.
5. Repeat step 4 for tubes #3-5 to serially dilute the malate standards. Do not add any malate to tube #6, which serves as a blank.
6. Obtain a 96-well test plate, prepare 2 replicates (A and B) of each malate standard by aliquoting 50 µL/well of each malate standard into duplicate wells of the 96-well test plate, following the plate format below:

	#1	#2	#3	#4	#5	#6
A	0.1 mM	0.05 mM	0.025 mM	0.0125 mM	0.00625 mM	blank
B	0.1 mM	0.05 mM	0.025 mM	0.0125 mM	0.00625 mM	blank

B. Preparation of test samples and blank

1. Cells or tissues can be homogenized in 4 volumes of the assay buffer (8648a). Centrifuge the samples at 10,000 ×g for 10 minutes at 4°C to remove insoluble material. The soluble fraction may be assayed directly.
2. Samples should be serially diluted to make sure the readings are within the detection limitation range. Prepare test samples to a final volume of 10 µL/well in a 96-well flat bottom plate.
3. Prepare a blank by adding 10 µL assay buffer (8648a) into one well of a 96-well flat bottom plate.

C. Working reagent preparation and measurements

1. Prepare appropriate volume of malate assay working reagent based on the number of samples to be measured. For each well of reaction, prepare working reagent by mixing 60 µL assay buffer (8648a), 10 µL developer solution (1X), 5 µL NAD (8648d), 5 µL WST solution, 5 µL cofactor (8648f), and 5 µL enzyme (8648g).
2. Add 90 µL of working reagent mix into each well of the 96-well plate containing malate standard, samples and blank. Measure the plate immediately at 440 nm with an ELISA plate reader to get A₀.
3. Incubate for 60 minutes at room temperature in dark. Read the absorbance at 440 nm with an ELISA plate reader to get A₆₀.

D. Calculations

1. Subtract the A_0 value from the A_{60} obtained with all other standard and samples to get ΔA_{60} value.
2. Subtract the ΔA_{60} value of the blank from the ΔA_{60} value obtained with all other standard and samples to get $\Delta\Delta A_{60}$ value.
3. Based on the calibrated $\Delta\Delta A_{60}$ of the malate standard, make a standard curve by plotting $\Delta\Delta A_{60}$ as a function of malate concentration (see Figure 1 for a typical standard curve). Determine the equation and R^2 value of the resulting trend line.
4. Suppose the equation of the trend line of the standard curve is $y = Ax + B$, calculate the malate concentration of test samples as follows:

$$[\text{Malate}] = \frac{\Delta\Delta A_{60} - B}{A}$$

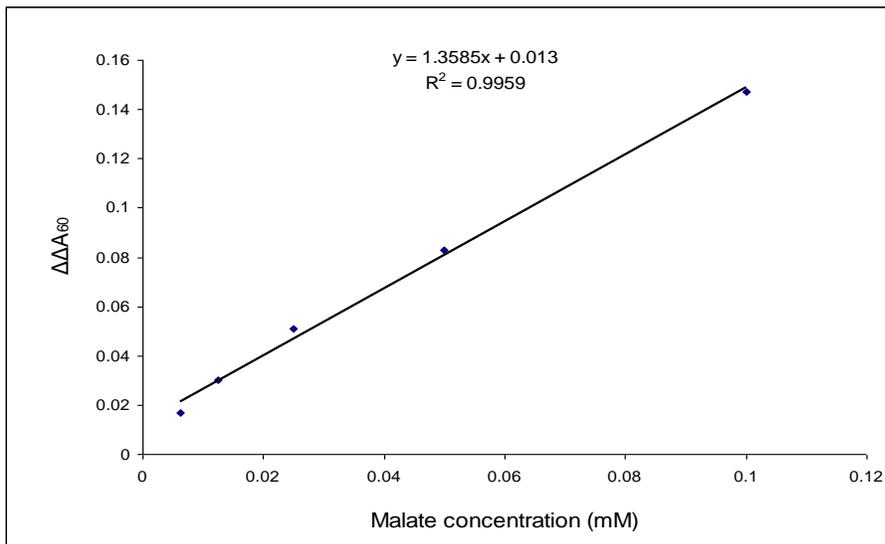


Figure1. A typical malate standard curve measured by ScienCell™ Malate Assay kit